

## A synergistic effect of albumin and H<sub>2</sub>O<sub>2</sub> accelerates corrosion of Ti6Al4V

Yu, Fei; Addison, Owen; Davenport, Alison J

DOI:

[10.1016/j.actbio.2015.07.046](https://doi.org/10.1016/j.actbio.2015.07.046)

License:

Creative Commons: Attribution-NonCommercial-NoDerivs (CC BY-NC-ND)

*Document Version*

Peer reviewed version

*Citation for published version (Harvard):*

Yu, F, Addison, O & Davenport, AJ 2015, 'A synergistic effect of albumin and H<sub>2</sub>O<sub>2</sub> accelerates corrosion of Ti6Al4V', *Acta Biomaterialia*, vol. 26, pp. 355-365. <https://doi.org/10.1016/j.actbio.2015.07.046>

[Link to publication on Research at Birmingham portal](#)

**Publisher Rights Statement:**

Checked for eligibility: 09/12/2015

**General rights**

Unless a licence is specified above, all rights (including copyright and moral rights) in this document are retained by the authors and/or the copyright holders. The express permission of the copyright holder must be obtained for any use of this material other than for purposes permitted by law.

- Users may freely distribute the URL that is used to identify this publication.
- Users may download and/or print one copy of the publication from the University of Birmingham research portal for the purpose of private study or non-commercial research.
- User may use extracts from the document in line with the concept of 'fair dealing' under the Copyright, Designs and Patents Act 1988 (?)
- Users may not further distribute the material nor use it for the purposes of commercial gain.

Where a licence is displayed above, please note the terms and conditions of the licence govern your use of this document.

When citing, please reference the published version.

**Take down policy**

While the University of Birmingham exercises care and attention in making items available there are rare occasions when an item has been uploaded in error or has been deemed to be commercially or otherwise sensitive.

If you believe that this is the case for this document, please contact [UBIRA@lists.bham.ac.uk](mailto:UBIRA@lists.bham.ac.uk) providing details and we will remove access to the work immediately and investigate.

## **A Synergistic Effect of Albumin and H<sub>2</sub>O<sub>2</sub> Accelerates Corrosion of Ti6Al4V**

Fei Yu<sup>a</sup>, Owen Addison<sup>b</sup> and Alison Davenport<sup>a</sup>

<sup>a</sup>School of Metallurgy and Materials, University of Birmingham, Birmingham, B15 2TT, UK.

<sup>b</sup>Biomaterials Unit, School of Dentistry, University of Birmingham, Birmingham, B4 6NN, UK,

Corresponding Author: Owen Addison,  
Biomaterials Unit,  
University of Birmingham School of Dentistry,  
St. Chad's Queensway,  
Birmingham,  
United Kingdom.

Telephone: 00 44 121 466 5506

Fax 00 44 121 466 5491

E-Mail: [o.addison@bham.ac.uk](mailto:o.addison@bham.ac.uk)

## **Abstract**

The synergistic effect of albumin and  $\text{H}_2\text{O}_2$  on corrosion of titanium alloy Ti6Al4V in physiological saline was investigated with long-term immersion tests and electrochemical methods. It was found that in the presence of both albumin and  $\text{H}_2\text{O}_2$ , the rate of metal release in immersion tests was far higher than in the presence of either species alone. Electrochemical polarisation curves and potentiostatic tests showed that  $\text{H}_2\text{O}_2$  increased both the rates of the anodic and cathodic reactions, while albumin significantly decreased the rate of the cathodic reaction and slightly decreased the rate of the anodic reaction. The synergistic effect of albumin and  $\text{H}_2\text{O}_2$  during immersion tests was attributed to the effect of adsorption of albumin in lowering the rate of the cathodic reaction and thus lowering the open circuit potential into the active region of titanium where complexation by  $\text{H}_2\text{O}_2$  increased the corrosion rate. The corrosion attack was found to be greater in the  $\beta$ -phase of the alloy. The findings suggest that current standard tests in physiological or phosphate-buffered saline may underestimate the rate of corrosion in the peri-implant environment, in which albumin is the predominant protein, and reactive oxygen species such as  $\text{H}_2\text{O}_2$  can occur as a result of inflammatory reactions in response to surgery, infection, or implant corrosion products.

## Introduction

Standard tests to study corrosion properties of biomedical alloys are typically carried out in solutions such as phosphate-buffered saline (PBS) [1-3] or physiological saline (0.9% NaCl) [4, 5]. However, the peri-implant environment contains a large range of biomolecules including proteins such as albumin [6] and products of cellular physiology such as reactive oxygen species (ROS) which includes hydrogen peroxide ( $H_2O_2$ ) [7, 8]. The effects of these species have been extensively investigated individually [9-20], but never in combination. In this paper, we show that a combination of albumin and  $H_2O_2$  can lead to much higher levels of corrosion of Ti6Al4V than either species alone, indicating the importance of developing tests that provide a more realistic simulation of the composition of the peri-implant environment.

Ti alloys are routinely used for biomedical applications because they have good biocompatibility, suitable mechanical properties and corrosion resistance [21]. However corrosion-related failures of implanted Ti devices have been recognised to occur *in-vivo* [22-24]; significantly elevated Ti levels have been detected in humans or animals with Ti implants [25-30]; and the analyses of peri-implant tissues and more distant tissues retrieved from patients with Ti implants have identified the presence of Ti species [31-36]. The biological consequences of the released Ti corrosion products are reported to include immunological responses leading to chronic inflammation around the implant which may ultimately lead to implant loss [22, 23, 32].

Ti implants are exposed to complex physiological environments that contain salts, lipids, proteins as well as living cells and/or bacteria which themselves can generate a variety of biomolecules in response to external stimulation [9, 37]. Local inflammation can occur around implants as a result of infection or indeed a result of the presence of debris derived

from the implant itself [22, 23]. Elemental analysis of oral mucosa surrounding Ti dental implants has demonstrated increased Ti release from the implant surfaces in inflamed sites when compared with healthy tissues although the exact mechanisms underpinning the observation were not determined [34]. During inflammation, levels of H<sub>2</sub>O<sub>2</sub> may become elevated being produced directly by bacteria (at levels which can exceed 5mM) or by immune cells which have migrated to the inflamed site [7, 8]. H<sub>2</sub>O<sub>2</sub> has been demonstrated to decrease the corrosion resistance of Ti implants [9-13] leading to surface roughening [13, 38] and the selective dissolution of the β phase of Ti6Al4V [39, 40]. This has been attributed to the complexation reaction between Ti and H<sub>2</sub>O<sub>2</sub>, and the structure of the corrosion product has been proposed as a strongly hydrated Ti(IV)-H<sub>2</sub>O<sub>2</sub> complex [41-44].

In addition following implantation, proteins quickly adsorb on the surface of an implant (e.g. Ti [45] and stainless steel [46]). Albumin is the most abundant protein found in blood (~4%) and in the extracellular environment, and its influence on the corrosion behaviour of metallic implants (including Ti) has been extensively reported [6, 14, 45-48]. However, the effect of albumin on the corrosion rate of Ti alloys is still unclear. Conflictingly, the presence of albumin has been reported to either decrease the corrosion rate of Ti alloys [15-17, 19, 49] or increase it [16, 18, 20] or have no effect [14, 50-52]. It is generally accepted that the addition of albumin decreases the cathodic reaction on Ti alloys, indicating that albumin serves as a cathodic inhibitor [14, 49, 51].

There are currently two papers where albumin and H<sub>2</sub>O<sub>2</sub> have both been mentioned in relation to Ti corrosion: in one paper on the effect of albumin, it was noted that H<sub>2</sub>O<sub>2</sub> is an intermediate species in the oxygen reduction reaction [16], and in another, it was noted that adsorption of albumin is higher on Ti surfaces previously exposed to H<sub>2</sub>O<sub>2</sub> [53]. However, there has been no systematic study of the synergistic interaction between H<sub>2</sub>O<sub>2</sub> and albumin on Ti corrosion, and all studies to date have studied the effects of the two species

independently. Accordingly in this paper we test the null hypothesis that the effects of  $H_2O_2$  and albumin on the corrosion of Ti6Al4V are unaltered by the combination of the two species.

## 1 Materials and Methods

### 1.1 Ti sample preparation

Ti6Al4V alloy (ASTM Grade 5) is a high strength  $\alpha/\beta$  alloy commonly used in orthopaedic, craniofacial and dental applications. Ti6Al4V discs (14 mm diameter and 1.2 mm thickness) were commercially sourced and machined by the supplier (Titanium Products Ltd, Solihull, UK).

For immersion tests, samples were mirror-polished on both sides according to a previously identified protocol [54], by first grinding with MD-Piano abrasive cloths (Struers, Ballerup, Denmark) in deionised water (Millipore, 18 M $\Omega$ ), followed by MD-Largo (Struers) with a 9  $\mu\text{m}$  diamond suspension. Finally the samples were polished with a MD-Chem polishing cloth (Struers) using 0.04  $\mu\text{m}$  OP-S Colloidal Silica suspension (Struers). All samples were thoroughly cleaned sequentially in acetone, ethanol, and deionised water, using ultrasonic agitation for 10 min at each stage. Specimens were finally dried in an air stream prior to use in further experiments.

For electrochemical tests, Ti discs were mounted in VARI-SET cold mounting acrylic (MetPrep Ltd, Coventry, UK) and used as the working electrode (WE, working area 1.5 cm<sup>2</sup>). To obtain a good reproducibility in electrochemical experiments, the time between polishing and electrochemical measurements was controlled: after final polishing with an MD-Chem polish cloth, the samples were immediately cleaned with deionised water, then dried in an air stream and left in open air for 5 min before immersing in test solutions.

## 1.2 Solutions

For immersion tests, H<sub>2</sub>O<sub>2</sub> (30% w/v, 30 g H<sub>2</sub>O<sub>2</sub> in 100 mL solution, BDH, England, UK) and bovine serum albumin ( $\geq 98\%$  (agarose gel electrophoresis) lyophilised powder, Sigma-Aldrich, Dorset, UK) was added to physiological saline (0.9% NaCl (Sigma-Aldrich, Dorset, UK), pH 6.7-7, 0.15 M). To minimise contamination with elements of interest for subsequent mass spectrometry measurements, ultrapure water (Gibco®, life technologies™, Paisley, UK) were used throughout for immersion tests.

For electrochemical tests, similar solutions were made using deionised water (Millipore, 18 M $\Omega$ ).

## 1.3 Immersion tests

All prepared mirror-polished Ti6Al4V samples were immersed in 2 mL of test solution in a 30 mL universal tube (transparent polystyrene with conical bottom) and sealed to prevent evaporation. For each experimental condition, three Ti samples were immersed and incubated at 37 °C. Samples were gently agitated on an A500 orbital mixer (Denley, UK) for 1 h per day. For each sample, the test medium was retrieved and replaced with new solutions following 7 days. Following 4 weeks of immersion, the retrieved solutions for each sample in the presence of different level of H<sub>2</sub>O<sub>2</sub> were pooled together for elemental concentration measurements.

The surfaces of the Ti6Al4V discs were characterised by scanning electron microscopy (SEM, JEOL 7000 (Jeol Ltd., Tokyo, Japan) using an accelerating voltage of 20 kV, a beam current of  $\sim 70 \mu\text{A}$ ) and energy dispersive X-ray spectroscopy (EDX, detector model: 7558, collecting window: ATW 2; acquisition time: 60 s; quantification method: standardless; Oxford



Instrument, UK). It was confirmed by EDX that  $\alpha$  phase contains  $6\pm 0.7$  wt% Al and  $2.5\pm 0.2$  wt% V and  $\beta$  phase contains  $4.2\pm 0.4$  wt% Al and  $9\pm 1.8$  wt% V.

Test solutions from each sample were syringe-filtered (Acrodisc<sup>®</sup> 32 mm syringe filter with  $0.45\ \mu\text{m}$  Supor<sup>®</sup> membrane, Pall Newquay, UK) and refrigerated at  $4\ ^\circ\text{C}$  prior to elemental concentration measurement. Elemental Ti, Al and V concentrations in the immersion solutions were quantified using Inductively Coupled Plasma Mass Spectrometry (ICP-MS) (Agilent 7500ce ICP-MS, Agilent Technologies, CA, USA) where the detectable limit for Ti, Al and V was  $0.2\ \text{ppb}$  ( $\text{ng/mL}$ ). One-way analyses of variance (ANOVA) and post-hoc Tukey tests were conducted to identify statistical differences ( $\alpha=0.05$ ) between ICP-MS quantifications of Ti, Al or V in immersion solutions containing varying concentrations of  $\text{H}_2\text{O}_2$  or varying concentrations of albumin.

#### **1.4 Electrochemical tests**

A standard three-electrode cell with reference electrode (RE), counter electrode (CE) and working electrode (WE) was used. The CE was a Pt mesh (working area  $\sim 4\ \text{cm}^2$ ) and the RE was a commercial saturated calomel electrode (SCE). The potential was controlled with a potentiostat (Model 1408, ACM Instruments, UK). The electrochemical cell was immersed in a water bath maintained at  $37\pm 1\ ^\circ\text{C}$ .

For polarisation curves, the open circuit potential (OCP) was measured for 1 h and then anodic and cathodic polarisation curves were performed. Anodic polarisation curves were measured by sweeping the potential from  $-50\ \text{mV}$  below the OCP to  $1200\ \text{mV}$  vs. SCE whilst the cathodic polarisation curves were measured separately by sweeping the potential from  $50\ \text{mV}$  above the OCP to  $-1400\ \text{mV}$  vs. SCE at a rate of  $1\ \text{mV/s}$ . Potentiostatic measurements were also performed following 1 h immersion at OCP. In addition, OCP of mirror-polished

Ti6Al4V in physiological saline with and without addition of H<sub>2</sub>O<sub>2</sub> and/or albumin were all monitored for 24 h. All electrochemical tests were performed at least twice for each condition, using a freshly polished sample and fresh solution in each case.

The surface morphology of samples was examined using both SEM and atomic force microscopy (AFM) in contact mode (Digital Instruments, Veeco Metrology Group; Model No.: MMAFMLN; California, USA) before and after the potentiostatic measurement in 10% H<sub>2</sub>O<sub>2</sub>. To easily locate the same region for comparison before and after exposure, one region of the mirror-polished sample was identified by an indentation mark (Vickers hardness test, load: 300 g, MVK-H1 hardness testing machine, Mitutoyo, Japan) which was then characterised by SEM. The carbon layer generated on the surface from SEM was removed by quickly (~10 s) polishing the sample on an MD-Chem polish cloth prior to cleaning as described above so that it would not affect the electrochemical experiments.

## 2 Results

### 2.1 Effect of H<sub>2</sub>O<sub>2</sub> on corrosion of Ti6Al4V

Figure 1 demonstrates that increased concentrations of Ti, Al and V were released from Ti6Al4V with increasing concentration of H<sub>2</sub>O<sub>2</sub>. For each element a one-way ANOVA demonstrated a significant impact of H<sub>2</sub>O<sub>2</sub> concentration on detected element release ( $p < 0.001$ ). More V was released than Al, especially following immersion in lower concentrations of H<sub>2</sub>O<sub>2</sub>. Ti, Al and V levels in the control solutions (no Ti disc) were negligible. Following Ti immersion, yellow precipitates were observed in the solution in 10% H<sub>2</sub>O<sub>2</sub> probably due to detachment of the surface corrosion product (Ti-H<sub>2</sub>O<sub>2</sub> complex [43]). Therefore, the Ti concentrations released from Ti6Al4V were not measured in 10% H<sub>2</sub>O<sub>2</sub> since the solid products would not be detected with the method used.

Figure 2 shows micrographs of the surface morphology of Ti6Al4V after immersion tests in physiological saline with different levels of H<sub>2</sub>O<sub>2</sub>. Figure 2a and Figure 2b show that in the absence of H<sub>2</sub>O<sub>2</sub> the surface was unattacked, and appeared similar to the as-polished surface. With increasing H<sub>2</sub>O<sub>2</sub> concentration the surfaces show signs of corrosion attack, particularly on the  $\beta$  phase, as well as formation of corrosion products on the surface.

The preferential attack of the  $\beta$  phase can be clearly seen in Figure 2k and Figure 2l following potentiostatic polarisation of Ti6Al4V at 600 mV for 30 min at 37 °C. The BSE image shows clear attack at the edge of  $\beta$  phase, while AFM shows that the whole  $\beta$  phase area was attacked to a depth of ~50 nm.

Figure 3a shows that the OCP increases with time following immersion and the values were almost 300 mV higher in the presence of H<sub>2</sub>O<sub>2</sub>. Figure 3b shows cathodic polarisation curves measured in physiological saline with and without H<sub>2</sub>O<sub>2</sub>. A cathodic current density plateau

was observed for Ti6Al4V under very negative potentials (less than -1 V vs. SCE) due to limited oxygen diffusion. With the addition of H<sub>2</sub>O<sub>2</sub>, the cathodic current densities were increased due to the reduction reaction of H<sub>2</sub>O<sub>2</sub>. It can also be seen that the cathodic current densities increased with increasing concentration of H<sub>2</sub>O<sub>2</sub> and the value of OCP moved to more positive values in the presence of H<sub>2</sub>O<sub>2</sub>, which is consistent with the OCP measurements in Figure 3a.

It can be seen from the anodic polarisation curves (Figure 3c) that Ti6Al4V showed passive behaviour in physiological saline and no significant change of anodic current density was observed up to a potential of 1200 mV vs. SCE. In the presence of H<sub>2</sub>O<sub>2</sub>, the anodic current densities became higher compared with those measured in physiological saline without H<sub>2</sub>O<sub>2</sub>. The anodic current densities increased with increasing concentration of H<sub>2</sub>O<sub>2</sub>. Furthermore the anodic current densities of Ti6Al4V in the presence of H<sub>2</sub>O<sub>2</sub> were slightly increased with increasing potential until an abrupt increase at 600-800 mV vs. SCE was observed, possibly due to oxygen evolution.

## **2.2 Effect of albumin on corrosion of Ti6Al4V**

Figure 4a demonstrates the OCP as a function of time for mirror-polished Ti6Al4V. The OCP increased with time and was almost 300 mV lower in the presence of albumin. The OCP of Ti6Al4V did not show significant differences in solutions containing different levels of albumin. Figure 4b shows that albumin addition significantly inhibited the cathodic reaction when compared with the cathodic reaction in physiological saline. The decreased cathodic current densities did not show significant differences in the solutions containing different levels of albumin. In addition, the OCP of Ti6Al4V moved to more negative values in the presence of albumin, which is consistent with OCP measurements in Figure 4a. The anodic current density was observed to be higher in the presence of albumin. This is possibly due to

the suppressed cathodic reaction. A particularly sharp active peak was found in 4% albumin (Figure 4d).

### 2.3 Effect of combination of H<sub>2</sub>O<sub>2</sub> and albumin on corrosion of Ti6Al4V

Figure 5 shows the concentrations of Ti, Al and V released from mirror-polished Ti6Al4V in the absence and presence of H<sub>2</sub>O<sub>2</sub> and albumin. Ti, Al and V levels in the control (without a Ti6Al4V disc) solutions were negligible, except for the Al level in the albumin control sample (15±10 ppb) (Figure 5) and it is possible that this was due to one contaminated sample. Of the three independent measurements, only one sample showed high Al level (26 ppb, 8 ppb and 10 ppb).

A significantly higher concentration of Ti was measured following immersion of the Ti samples in the presence of H<sub>2</sub>O<sub>2</sub> when compared with H<sub>2</sub>O<sub>2</sub>-free solution ( $p < 0.01$ ) and similar to the 4 week immersion tests (see Figure 1), the amount of released V was greater than Al. In the presence of albumin, a small increase ( $p < 0.01$ ) in the measured Ti concentration (65±5 ppb) was observed when compared with the (albumin-free) physiological saline control. Immersion in mixed solutions of H<sub>2</sub>O<sub>2</sub> and albumin resulted in a substantial increase in the release of Ti, Al and V ( $p < 0.001$  for each element), which increased with the increasing concentration of albumin in the mixed solutions. The concentration of Al measured in the mixed solutions was greater than that in the presence of H<sub>2</sub>O<sub>2</sub> without albumin ( $p < 0.01$ ).

Figure 6 shows that the corrosion products on the Ti6Al4V surface appeared porous in the presence of H<sub>2</sub>O<sub>2</sub> based on the secondary electron (SE) image, and the  $\beta$  phase appeared to be preferentially attacked based on the backscatter electron (BSE) image, which was similar to the observation following the 4 week immersion tests in H<sub>2</sub>O<sub>2</sub> (Figure 2). Figure 6 also shows

that the surface of Ti6Al4V after immersion in albumin did not show a significant difference from the sample immersed in physiological saline alone. However, after immersion in the mixed solutions of H<sub>2</sub>O<sub>2</sub> and albumin the surface of Ti6Al4V was relatively smooth with no obvious corrosion products and the  $\beta$  phase was preferentially attacked. Figure 7a shows the OCP as a function of time for mirror-polished Ti6Al4V in the absence and presence of H<sub>2</sub>O<sub>2</sub> and albumin. The OCP was higher in the presence of H<sub>2</sub>O<sub>2</sub> compared with (H<sub>2</sub>O<sub>2</sub>-free) physiological saline, and was lower after the addition of albumin. The OCP was lower in the presence of albumin compared with (albumin-free) physiological saline, and was higher after the addition of H<sub>2</sub>O<sub>2</sub>. The OCP of Ti6Al4V in the presence of mixed solutions of H<sub>2</sub>O<sub>2</sub> and albumin was close to that in the physiological saline control. In addition, the OCP was not found to depend on the concentration of albumin in the mixed solutions.

Figure 7b shows cathodic polarisation curves for mirror-polished Ti6Al4V in the absence and presence of H<sub>2</sub>O<sub>2</sub> and albumin. It can be seen that the addition of albumin decreased the cathodic current density in the presence of H<sub>2</sub>O<sub>2</sub> alone, and the addition of H<sub>2</sub>O<sub>2</sub> increased the cathodic current density in the presence of albumin alone.

For anodic polarisation curves (Figure 7c), Ti6Al4V exhibited higher anodic current densities in mixed solutions of H<sub>2</sub>O<sub>2</sub> and albumin compared with physiological saline, and this appears to be mainly due to an enhanced anodic reaction. In addition, the anodic current densities of Ti6Al4V in mixed solutions were increased with an increasing concentration of albumin (Figure 7d), which is consistent with the metal release results (Figure 5). The anodic current density of Ti6Al4V showed an abrupt increase in the presence of mixed solutions at  $600 \pm 80$  mV vs. SCE, which was similar to that observed in H<sub>2</sub>O<sub>2</sub> (see Section 3.1.3.1) and is possibly due to oxygen evolution.

Figure 8 illustrates the potentiostatic measurements of mirror-polished Ti6Al4V in physiological saline with addition of albumin and/or H<sub>2</sub>O<sub>2</sub> at different potentials. The solution was stirred at ~1000 s intervals to ensure complete mixing. H<sub>2</sub>O<sub>2</sub> and/or albumin were added just prior to stirring for some of the measurements. Figure 8a demonstrates that the cathodic steady state current densities of Ti6Al4V at -800 mV vs. SCE were decreased following addition of albumin at the 1st ~1000 s interval, consistent with the cathodic polarisation results (Figure 4b). It can also be seen that the cathodic steady state current densities in the absence and presence of albumin were increased after addition of H<sub>2</sub>O<sub>2</sub> at the 2nd ~1000 s interval, consistent with the cathodic polarisation results in Figure 7b. In addition, the cathodic steady state current densities in H<sub>2</sub>O<sub>2</sub>-containing solution were decreased following addition of albumin at the 3rd ~1000 s interval, which is also consistent with the cathodic polarisation results (Figure 7b).

Figure 8b and Figure 8c show that the anodic steady state current densities of Ti6Al4V at both anodic potentials decreased after addition of albumin at the 1st ~1000 s interval. It has also been shown that at the 2nd ~1000 s interval, the anodic steady state current densities in the absence and presence of albumin were increased after addition of H<sub>2</sub>O<sub>2</sub>. In addition, at the 3rd ~1000 s interval, the anodic steady state current densities in the presence of H<sub>2</sub>O<sub>2</sub> were also decreased after addition of albumin.

Figure 9 shows the OCP as a function of time for 24 h for mirror-polished Ti6Al4V in physiological saline with and without H<sub>2</sub>O<sub>2</sub> and albumin. The solution was stirred at intervals to ensure complete mixing. H<sub>2</sub>O<sub>2</sub> or albumin was added just prior to stirring at ~1 h or ~4 h for some of the measurements. At ~1 h following addition of H<sub>2</sub>O<sub>2</sub>, the OCP of Ti6Al4V shifted to a higher value when compared with the OCP in physiological saline alone. At ~4 h when albumin was added into the H<sub>2</sub>O<sub>2</sub>-containing solution, the OCP decreased and this was consistent with the 1 h OCP measurement (Figure 7a). At ~1 h following addition of

albumin, the OCP of Ti6Al4V decreased when compared with the OCP measured in physiological saline alone. Subsequently at ~4 h when H<sub>2</sub>O<sub>2</sub> was added into the albumin-containing solution, the OCP of Ti6Al4V increased, which again was consistent with the 1 h OCP measurement (Figure 7a). After 24 h exposure, Ti6Al4V exhibited the highest OCP value in H<sub>2</sub>O<sub>2</sub> and the lowest in albumin whilst the OCP in mixed solutions was close to that in physiological saline, which also agreed with the previous observations (see Figure 7a).



### **3 Discussion**

#### **3.1 Effect of H<sub>2</sub>O<sub>2</sub> on corrosion of Ti6Al4V**

Ti6Al4V is highly resistant to corrosion in physiological saline: it can be seen from Figure 1 that the concentrations of Ti, Al and V measured in the control solutions were negligible. However, the concentrations of released metal ions (Figure 1) and anodic current densities measured in polarisation curves (Figure 3) increased with the increasing concentration of H<sub>2</sub>O<sub>2</sub>, indicating decreased corrosion resistance of Ti6Al4V in the presence of H<sub>2</sub>O<sub>2</sub>, which is consistent with previous studies on Ti alloys [10-13, 55] and has been explained in terms of the complexation of Ti by H<sub>2</sub>O<sub>2</sub> [41-44].

Since all experiments were carried out under naturally-aerated conditions, it is assumed that the cathodic reaction in physiological saline is oxygen reduction. However, in the presence of H<sub>2</sub>O<sub>2</sub> the cathodic reaction is likely to be dominated by the reduction reaction of H<sub>2</sub>O<sub>2</sub> since H<sub>2</sub>O<sub>2</sub> is a strong oxidiser and has a high standard reduction potential ( $E^\circ = 1.54 \text{ V vs. SCE}$ ) [56], leading to a higher cathodic current density and also resulting in a more positive OCP.

#### **3.2 Effect of albumin on corrosion of Ti6Al4V**

It can be seen that the presence of albumin significantly inhibits the cathodic reaction of Ti6Al4V (Figure 4 and Figure 8), resulting in a lower OCP (Figure 4), consistent with previous studies on Ti alloys [14, 51]. It has been proposed that albumin strongly adsorbs on the surfaces of metals including Ti by chemisorption through carboxylate/amino group or through electrostatic interactions, blocking electrochemical reactions [14, 45, 57].

In the current study, the anodic steady state current density under potentiostatic conditions decreased following addition of albumin (Figure 8), indicating that the anodic reaction was suppressed. Similar observations have been made on CP-Ti [14] and Ti6Al4V-ELI [16]. It is possible that the adsorption of albumin also inhibits the anodic reaction of Ti6Al4V, resulting in a lower anodic steady state current. Therefore, the observed higher net anodic current densities in polarisation curves in the presence of albumin (Figure 4) are more likely to be due to the suppressed cathodic reaction.

It is known that Ti may show an “active” peak at low potential. This has been attributed to the formation of  $Ti^{3+}$  [58]. A particularly sharp active peak was found in the presence of 4% albumin (Figure 7), which has not been previously reported. It should be noted that in previous studies [17, 19, 51], polarisation curves started from very low potentials (e.g. -1 V vs Ag/AgCl [51]), whereas in the current study, anodic and cathodic polarisation tests were conducted separately to reduce the effect of prior cathodic polarisation on anodic polarisation and vice versa. The history of cathodic reaction may have an influence on anodic behaviour of Ti6Al4V during the polarisation tests.

A small increase in Ti release from Ti6Al4V was observed in the presence of albumin after the immersion test (Figure 5). However, the presence of albumin inhibited the cathodic and anodic reactions in physiological saline. Similar apparently contradictory results can be found in the work of Padilla and Bronson [16] and Karimi and Alfantazi [17-20]. The most likely explanation is that the lower OCP brought about by the suppressed cathodic reaction may drive the dissolution of Ti6Al4V into the “active” region, so the presence of albumin increases the corrosion rate of Ti6Al4V at the open circuit potential.

### 3.3 Effect of the combination of albumin and H<sub>2</sub>O<sub>2</sub> on corrosion of Ti6Al4V

It can be seen from Figure 7 that the cathodic current density is lower in the presence of both H<sub>2</sub>O<sub>2</sub> and albumin when compared with those in H<sub>2</sub>O<sub>2</sub> alone, suggesting that the presence of albumin inhibits the cathodic reaction of Ti6Al4V in H<sub>2</sub>O<sub>2</sub>-containing solutions. In polarisation curves (Figure 7) higher net anodic current densities were observed in the presence of mixed solutions when compared with those in the presence of H<sub>2</sub>O<sub>2</sub> alone: this is likely to be due to the suppressed cathodic reaction. Potentiostatic studies showed that the anodic steady state current densities (Figure 8) in the presence of H<sub>2</sub>O<sub>2</sub> were decreased after addition of albumin, indicating that the presence of albumin suppressed anodic reaction of Ti6Al4V in H<sub>2</sub>O<sub>2</sub>-containing solutions.

A considerably higher rate of metal release from Ti6Al4V was observed in mixed solutions compared with that in either albumin or H<sub>2</sub>O<sub>2</sub> alone after immersion tests (Figure 5), which has not previously been reported. This attack was found to be greater in the  $\beta$ -phase of the alloy (Figure 6). The most likely explanation is that the cathodic reaction is suppressed by the addition of albumin, taking the potential of Ti6Al4V into the active region, thereby increasing the rate of corrosion. Figure 10 shows a diagram to explain this hypothesis. The anodic and cathodic reactions in the absence of H<sub>2</sub>O<sub>2</sub> and albumin are shown by the thin black lines. The anodic and cathodic reactions intersect in the passive region at point A. Addition of albumin to physiological saline (thick green lines) slightly decreases the anodic reaction and greatly inhibits the cathodic reaction; the anodic and cathodic curves intersect in the active region below the peak at point B, giving a slightly higher corrosion rate (Figure 5) and lower OCP (Figure 9). Addition of H<sub>2</sub>O<sub>2</sub> to physiological saline (thin dashed blue lines) substantially increases both the anodic and cathodic reactions, with the intersection at point C in the passive region, giving a higher OCP (Figure 9) and higher corrosion rate (Figure 5).

With addition of both  $\text{H}_2\text{O}_2$  and albumin to physiological saline (thick dashed red lines), the anodic reaction is slightly lower than with  $\text{H}_2\text{O}_2$  alone, and the cathodic reaction is also lower than that with  $\text{H}_2\text{O}_2$  alone, but the lines intersect in the active region (point D) so the OCP is similar to that physiological saline in the absence of  $\text{H}_2\text{O}_2$  and albumin (Figure 9), but the corrosion rate is much higher (Figure 5).

The results presented in this paper show that addition of both  $\text{H}_2\text{O}_2$  and albumin to physiological saline leads to a far higher rate of corrosion of Ti6Al4V than that in physiological saline alone. Albumin is the most common protein in the peri-implant environment and ROS such as  $\text{H}_2\text{O}_2$  are produced in the presence of inflammation reaction [7, 8], which are common after surgery, or in response to infection or corrosion products. However, current standard tests for biomedical alloys use saline solutions e.g. PBS and 0.9% NaCl [1-5], in which far lower corrosion rates are observed. The considerable increase in corrosion rate observed in the current work in the presence of both albumin and  $\text{H}_2\text{O}_2$  suggests that current standard tests may underestimate the true rate of corrosion of implants in the body, and that testing should take place in solutions that more closely simulate the peri-implant environment to take account of the synergistic effect of albumin and  $\text{H}_2\text{O}_2$  (or other ROS) in promoting corrosion of Ti6Al4V.

#### **4 Conclusions**

1. The presence of  $\text{H}_2\text{O}_2$  promotes corrosion of Ti6Al4V by increasing both anodic and cathodic reactions, leading to increasing release of Ti, Al and V with increasing concentration of  $\text{H}_2\text{O}_2$  in physiological saline.
2. The presence of albumin strongly inhibits the cathodic reaction and slightly inhibits the anodic reaction of Ti6Al4V in physiological saline resulting in a lower OCP. During

anodic polarisation, a net active peak is observed following addition of albumin owing to suppression of the cathodic reaction. The presence of albumin causes a small increase in Ti release from Ti6Al4V in long-term immersion tests, which is attributed to the decrease OCP brought about by the inhibited cathodic reaction, leading to dissolution of Ti6Al4V in the active region.

3. In the presence of both H<sub>2</sub>O<sub>2</sub> and albumin, there is a very much higher rate of metal release from Ti6Al4V compared with that in physiological saline alone. This can be attributed to an increased rate of the anodic reaction caused by H<sub>2</sub>O<sub>2</sub> complexation of Ti and some suppression of cathodic reaction by adsorption of albumin, leading to a OCP in the active region of Ti6Al4V and a correspondingly high corrosion rate.

4. The corrosion attack was found to be greater in the β-phase of Ti6Al4V.

5. Standard tests that currently use physiological or phosphate-buffered saline may underestimate the rate of corrosion of Ti in the body since they neglect the synergistic effects of albumin and reactive oxygen species such as H<sub>2</sub>O<sub>2</sub> that are found in peri-implant tissue.

## **Acknowledgement**

Dr F Yu has been funded in part by the University of Birmingham and the China Scholarship Council. Prof O Addison is funded by NIHR Clinician Scientist Award NIHR/CS/010/001.

## **Disclosures**

The authors have no conflicts of interest to declare.

## References

- [1] ASTM F2129-15 Standard test method for conducting cyclic potentiodynamic polarization measurements to determine the corrosion susceptibility of small implant devices (2015). ASTM International, West Conshohocken, United States.
- [2] ASTM F3044-14 Test method for standard test method for evaluating the potential for galvanic corrosion for medical implants (2014). ASTM International, West Conshohocken, United States.
- [3] ASTM F746-04 Standard test method for pitting or crevice corrosion of metallic surgical implant materials (2014).
- [4] ASTM F1801-97 Standard practice for corrosion fatigue testing of metallic implant materials (2014). ASTM International, West Conshohocken, United States.
- [5] ASTM F1875-98 Standard practice for fretting corrosion testing of modular implant interfaces: Hip femoral head-bore and cone taper interface (2014). ASTM International, West Conshohocken, United States.
- [6] Francis GL. Albumin and mammalian cell culture: implications for biotechnology applications. *Cytotechnology* 2010;62:1-16.
- [7] Test ST, Weiss SJ. Quantitative and temporal characterization of the extracellular H<sub>2</sub>O<sub>2</sub> pool generated by human neutrophils. *J Biol Chem* 1984;259:399-405.
- [8] Robinson JM. Reactive oxygen species in phagocytic leukocytes. *Histochem Cell Biol* 2008;130:281-97.
- [9] Mabillean G, Bourdon S, Joly-Guillou ML, Filmon R, Basle MF, Chappard D. Influence of fluoride, hydrogen peroxide and lactic acid on the corrosion resistance of commercially pure titanium. *Acta Biomater* 2006;2:121-9.
- [10] Pan J, Thierry D, Leygraf C. Hydrogen peroxide toward enhanced oxide growth on titanium in PBS solution: Blue coloration and clinical relevance. *J Biomed Mater Res* 1996;30:393-402.
- [11] Pan J, Thierry D, Leygraf C. Electrochemical impedance spectroscopy study of the passive oxide film on titanium for implant application. *Electrochim Acta* 1996;41:1143-53.
- [12] Al-Mobarak NA, Al-Mayouf AM, Al-Swayih AA. The effect of hydrogen peroxide on the electrochemical behavior of Ti and some of its alloys for dental applications. *Mater Chem Phys* 2006;99:333-40.
- [13] Fonseca C, Barbosa MA. Corrosion behaviour of titanium in biofluids containing H<sub>2</sub>O<sub>2</sub> studied by electrochemical impedance spectroscopy. *Corros Sci* 2001;43:547-59.
- [14] Cheng XL, Roscoe SG. Corrosion behavior of titanium in the presence of calcium phosphate and serum proteins. *Biomaterials* 2005;26:7350-6.
- [15] Khan MA, Williams RL, Williams DF. The corrosion behaviour of Ti-6Al-4V, Ti-6Al-7Nb and Ti-13Nb-13Zr in protein solutions. *Biomaterials* 1999;20:631-7.
- [16] Padilla N, Bronson A. Electrochemical characterization of albumin protein on Ti-6Al-4V alloy immersed in a simulated plasma solution. *J Biomed Mater Res A* 2007;81A:531-43.
- [17] Karimi S, Nickchi T, Alfantazi A. Effects of bovine serum albumin on the corrosion behaviour of AISI 316L, Co-28Cr-6Mo, and Ti-6Al-4V alloys in phosphate buffered saline solutions. *Corros Sci* 2011;53:3262-72.
- [18] Karimi S, Nickchi T, Alfantazi AM. Long-term corrosion investigation of AISI 316L, Co-28Cr-6Mo, and Ti-6Al-4V alloys in simulated body solutions. *Appl Surf Sci* 2012;258:6087-96.
- [19] Karimi S, Alfantazi AM. Electrochemical corrosion behavior of orthopedic biomaterials in presence of human serum albumin. *J Electrochem Soc* 2013;160:C206-C14.

- [20] Karimi S, Alfantazi AM. Ion release and surface oxide composition of AISI 316L, Co-28Cr-6Mo, and Ti-6Al-4V alloys immersed in human serum albumin solutions. *Mater Sci Eng C Mater Biol Appl* 2014;40:435-44.
- [21] Liu XY, Chu PK, Ding CX. Surface modification of titanium, titanium alloys, and related materials for biomedical applications. *Mater Sci Eng R* 2004;47:49-121.
- [22] Hallam P, Haddad F, Cobb J. Pain in the well-fixed, aseptic titanium hip replacement - The role of corrosion. *J Bone Joint Surg Br* 2004;86B:27-30.
- [23] Thomas SR, Shukla D, Latham PD. Corrosion of cemented titanium femoral stems. *J Bone Joint Surg Br* 2004;86B:974-8.
- [24] Cadosch D, Chan E, Gautschi OP, Filgueira L. Metal is not inert: Role of metal ions released by biocorrosion in aseptic loosening-Current concepts. *J Biomed Mater Res A* 2009;91A:1252-62.
- [25] Sarmiento-Gonzalez A, Encinar JR, Marchante-Gayon JM, Sanz-Medel A. Titanium levels in the organs and blood of rats with a titanium implant, in the absence of wear, as determined by double-focusing ICP-MS. *Anal Bioanal Chem* 2009;393:335-43.
- [26] Sarmiento-Gonzalez A, Marchante-Gayon JM, Tejerina-Lobo JM, Paz-Jimenez J, Sanz-Medel A. High-resolution ICP-MS determination of Ti, V, Cr, Co, Ni, and Mo in human blood and urine of patients implanted with a hip or knee prosthesis. *Anal Bioanal Chem* 2008;391:2583-9.
- [27] Jacobs JJ, Skipor AK, Patteson LM, Hallab NJ, Paprosky WG, Black J, Galante JO. Metal release in patients who have has a primary total hip arthroplasty - A prospective, controlled, longitudinal study. *J Bone Joint Surg Am* 1998;80A:1447-58.
- [28] Kasai Y, Iida R, Uchida A. Metal concentrations in the serum and hair of patients with titanium alloy spinal implants. *Spine* 2003;28:1320-6.
- [29] Boyer P, Lazennec J-Y, Poupon J, Rousseau M-A, Ravaud P, Catonne Y. Clinical and biological assessment of cemented titanium femoral stems: an 11-year experience. *Int Orthop* 2009;33:1209-15.
- [30] Rubio JC, Garcia-Alonso MC, Alonso C, Alobera MA, Clemente C, Munuera L, Escudero ML. Determination of metallic traces in kidneys, livers, lungs and spleens of rats with metallic implants after a long implantation time. *J Mater Sci Mater Med* 2008;19:369-75.
- [31] Uo M, Asakura K, Yokoyama A, Ishikawa M, Tamura K, Totsuka Y, Akasaka T, Watari F. X-ray absorption fine structure (XAFS) analysis of titanium-implanted soft tissue. *Dent Mater J* 2007;26:268-73.
- [32] Addison O, Davenport AJ, Newport RJ, Kalra S, Monir M, Mosselmans JFW, Proops D, Martin RA. Do 'passive' medical titanium surfaces deteriorate in service in the absence of wear? *J Royal Soc Interface* 2012;9:3161-4.
- [33] Jacobs JJ, Gilbert JL, Urban RM. Current concepts review - corrosion of metal orthopaedic implants. *Bone Joint J* 1998;80:268-82.
- [34] Olmedo DG, Nalli G, Verdu S, Paparella ML, Cabrini RL. Exfoliative cytology and titanium dental implants: a pilot study. *J Periodontol* 2013;84:78-83.
- [35] Olmedo DG, Paparella ML, Brandizzi D, Cabrini RL. Reactive lesions of peri-implant mucosa associated with titanium dental implants: a report of 2 cases. *Int J Oral Maxillofac Surg* 2010;39:503-7.
- [36] Olmedo DG, Paparella ML, Spielberg M, Brandizzi D, Guglielmotti MB, Cabrini RL. Oral mucosa tissue response to titanium cover screws. *J Periodontol* 2012;83:973-80.
- [37] Hanawa T. Metal ion release from metal implants. *Mater Sci Eng C* 2004;24:745-52.
- [38] Fadl-Allah SA, El-Sherief RM, Badawy WA. Electrochemical formation and characterization of porous titania TiO<sub>2</sub> films on Ti. *J Appl Electrochem* 2008;38:1459-66.
- [39] Gilbert JL. Method of preparing biomedical surface. Patent #8,012,338 September 6, 2011.



- [40] Chandrasekaran N, Bai Z, Gilbert JL. Titanium electrochemistry in the presence of the inflammatory species H<sub>2</sub>O<sub>2</sub>. Translation society for biomaterials annual meeting 2006.
- [41] Tengvall P, Bertilsson L, Liedberg B, Elwing H, Lundstrom I. Degradation of dried ti-peroxy gels made from metallic titanium and hydrogen-peroxide. *J Colloid Interface Sci* 1990;139:575-80.
- [42] Tengvall P, Elwing H, Lundstrom I. Titanium gel made from metallic titanium and hydrogen-peroxide. *J Colloid Interface Sci* 1989;130:405-13.
- [43] Tengvall P, Elwing H, Sjoqvist L, Lundstrom I, Bjursten LM. Interaction between hydrogen-peroxide and titanium - a possible role in the biocompatibility of titanium. *Biomaterials* 1989;10:118-20.
- [44] Tengvall P, Lundstrom I, Sjoqvist L, Elwing H, Bjursten LM. Titanium-hydrogen peroxide interaction - model studies of the influence of the inflammatory response on titanium implants. *Biomaterials* 1989;10:166-75.
- [45] Jackson DR, Omanovic S, Roscoe SG. Electrochemical studies of the adsorption behavior of serum proteins on titanium. *Langmuir* 2000;16:5449-57.
- [46] Omanovic S, Roscoe SG. Electrochemical studies of the adsorption behavior of bovine serum albumin on stainless steel. *Langmuir* 1999;15:8315-21.
- [47] Wang LN, Huang XQ, Shinbine A, Luo JL. Influence of albumin on the electrochemical behaviour of Zr in phosphate buffered saline solutions. *J Mater Sci Mater Med* 2013;24:295-305.
- [48] Wang W, Mohammadi F, Alfantazi A. Corrosion behaviour of niobium in phosphate buffered saline solutions with different concentrations of bovine serum albumin. *Corros Sci* 2012;57:11-21.
- [49] Mareci D, Chelariu R, Gordin D-M, Ungureanu G, Gloriant T. Comparative corrosion study of Ti-Ta alloys for dental applications. *Acta Biomater* 2009;5:3625-39.
- [50] Huang HH, Lee TH. Electrochemical impedance spectroscopy study of Ti-6Al-4V alloy in artificial saliva with fluoride and/or bovine albumin. *Dent Mater* 2005;21:749-55.
- [51] Hiromoto S, Mischler S. The influence of proteins on the fretting-corrosion behaviour of a Ti6Al4V alloy. *Wear* 2006;261:1002-11.
- [52] Ban S, Hasegawa J, Maruno S. Electrochemical corrosion behavior of hydroxyapatite glass titanium composite. *Biomaterials* 1991;12:205-9.
- [53] Nagassa ME, Daw AE, Rowe WG, Carley A, Thomas DW, Moseley R. Optimisation of the hydrogen peroxide pre-treatment of titanium: surface characterisation and protein adsorption. *Clin Oral Implants Res* 2008;19:1317-26.
- [54] Yu F, Addison O, Baker SJ, Davenport AJ. Lipopolysaccharide inhibits or accelerates biomedical titanium corrosion depending on environmental acidity. *Int J Oral Sci* 2015:1-8.
- [55] Brooks E, Tobias M, Krautsak K, Ehrensberger M. The influence of cathodic polarization and simulated inflammation on titanium electrochemistry. *J Biomed Mater Res Part B Appl Biomater* 2014;102:1445-53.
- [56] Pourbaix M. Atlas of electrochemical equilibria in aqueous solutions. Houston: TX. NACE; 1974.
- [57] Klinger A, Steinberg D, Kohavi D, Sela MN. Mechanism of adsorption of human albumin to titanium in vitro. *J Biomed Mater Res* 1997;36:387-92.
- [58] Yu SY, Scully JR. Corrosion and passivity of Ti-13% Nb-13% Zr in comparison to other biomedical implant alloys. *Corrosion* 1997;53:965-76.

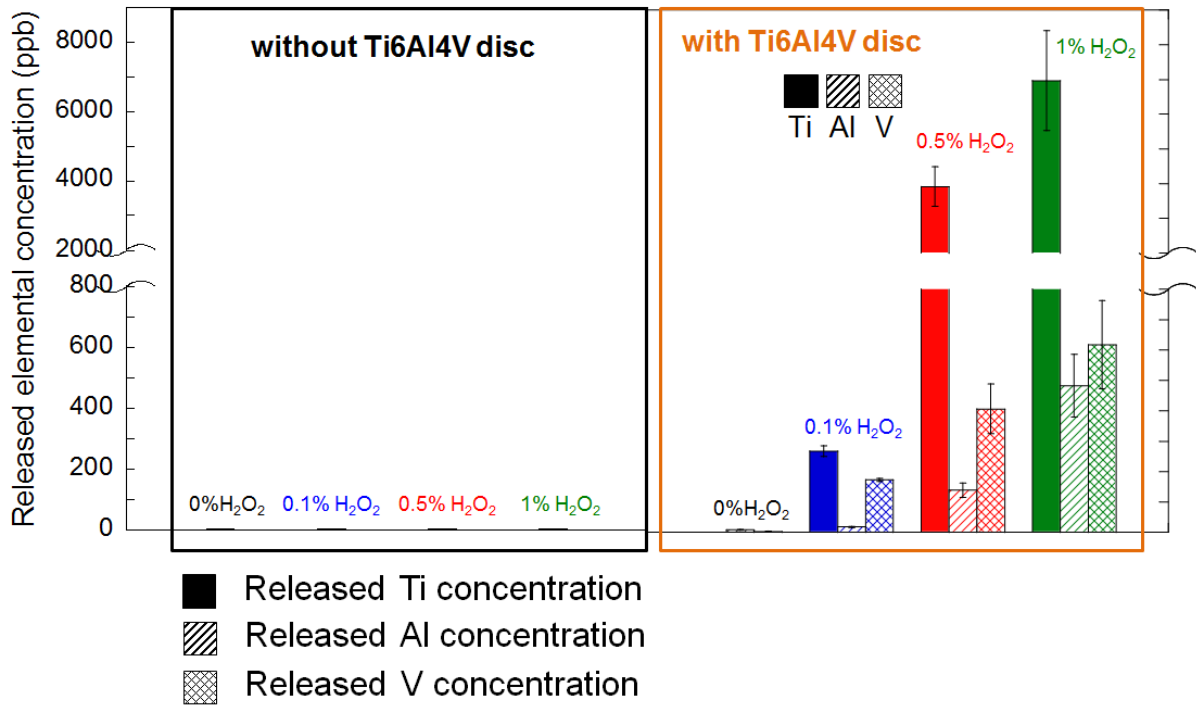


Figure 1 The mean concentrations (ppb) measured with ICP-MS of Ti, Al and V released from mirror-polished Ti6Al4V following immersion in physiological saline (0.15 M NaCl) with and without different levels of H<sub>2</sub>O<sub>2</sub> for 4 weeks at 37 °C. Error bars refer to 1 standard deviation (n=3).

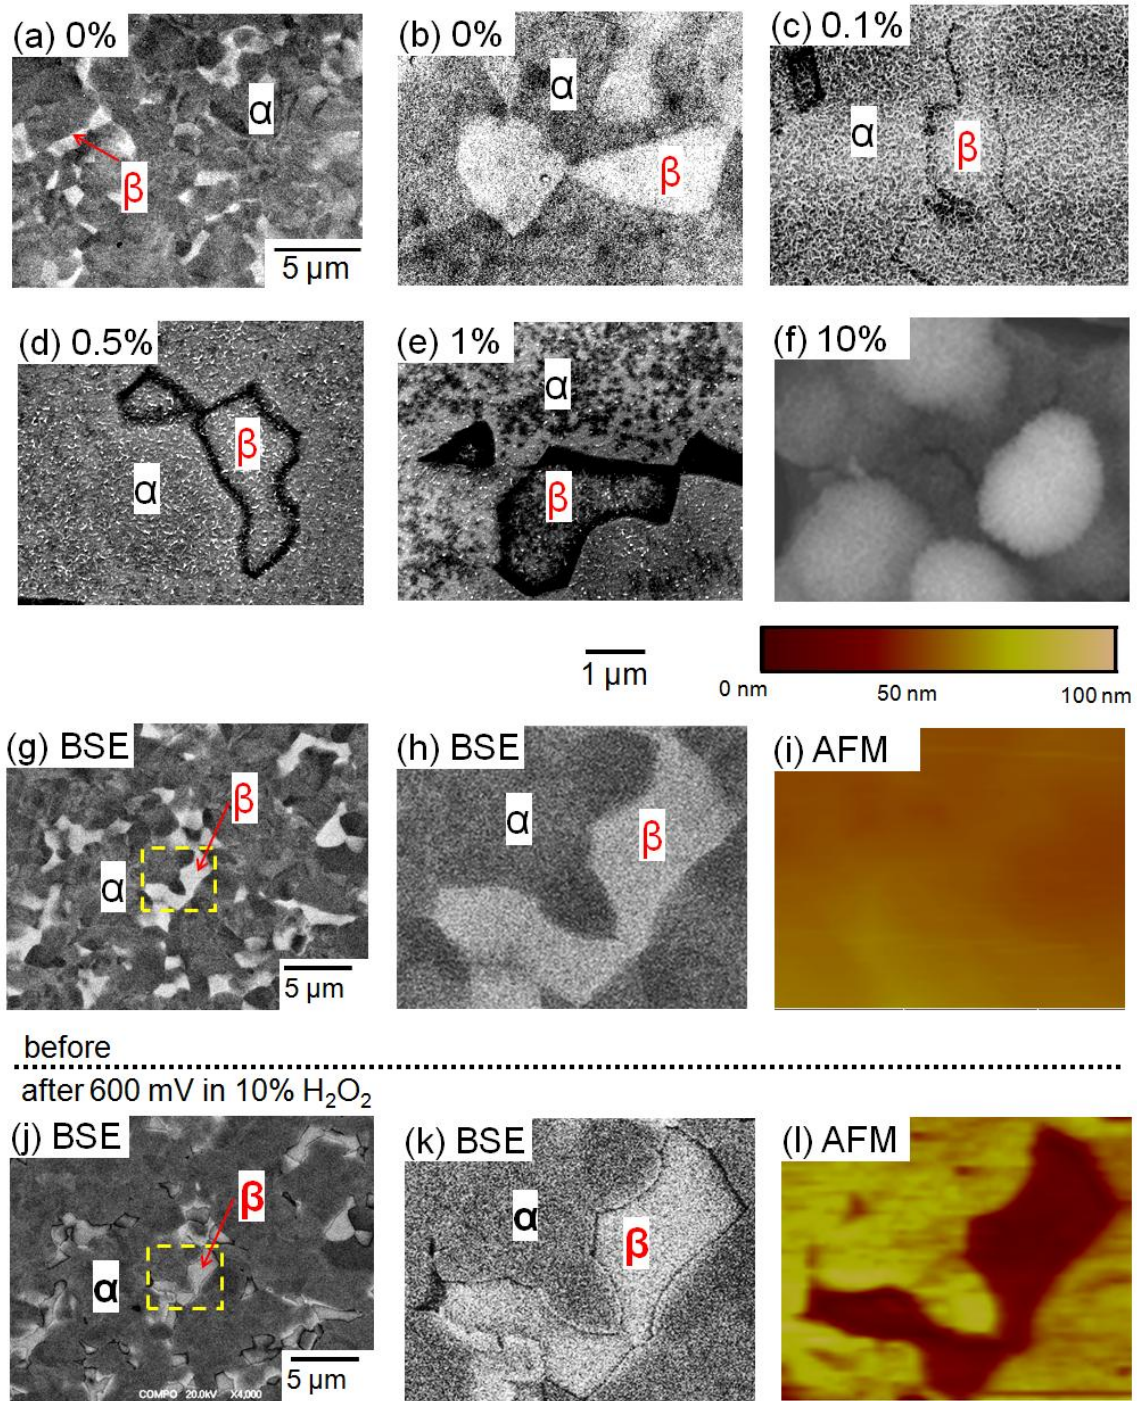


Figure 2 (a-f) surface morphologies of mirror-polished Ti6Al4V following immersion in physiological saline (0.15 M NaCl) with and without different levels of H<sub>2</sub>O<sub>2</sub> for 4 weeks at 37 °C; surface morphology/topography of (g-i) before and (j-l) after potentiostatic measurement in 10% H<sub>2</sub>O<sub>2</sub>-containing physiological saline at 600 mV vs. SCE for 30 min at 37 °C. BSE: backscatter electron SEM image. Note that all micrographs are at the same scale except (a, g, j) which are at lower magnification as indicated.  $\alpha$  phase and  $\beta$  phase were identified with EDX (data not shown) and BSE.

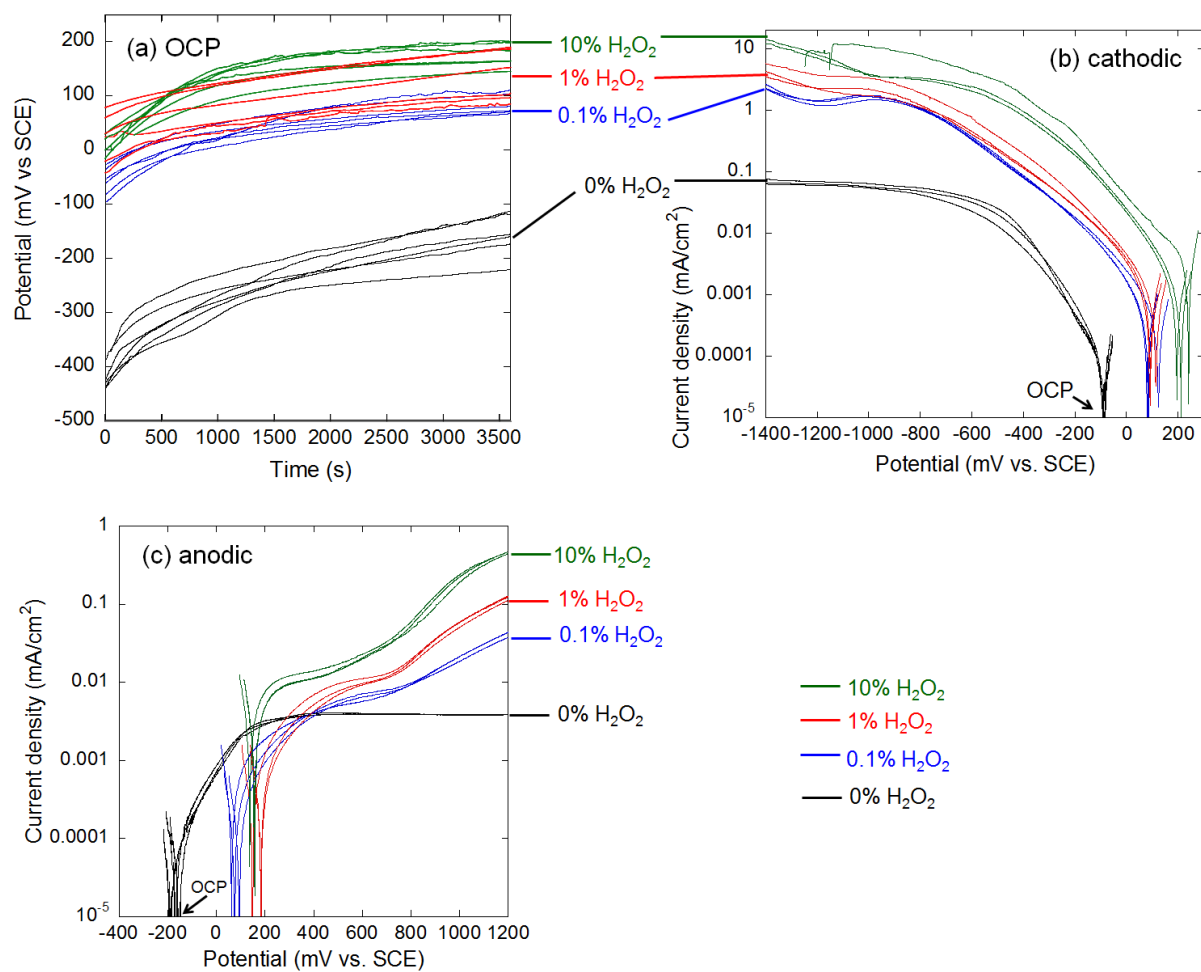


Figure 3 (a) OCP as a function of time; (b) cathodic and (c) anodic polarisation curves for mirror-polished Ti6Al4V in physiological saline (0.15 M NaCl) with and without different levels of H<sub>2</sub>O<sub>2</sub> at 37 °C. The sweep rate was 1 mV/s.

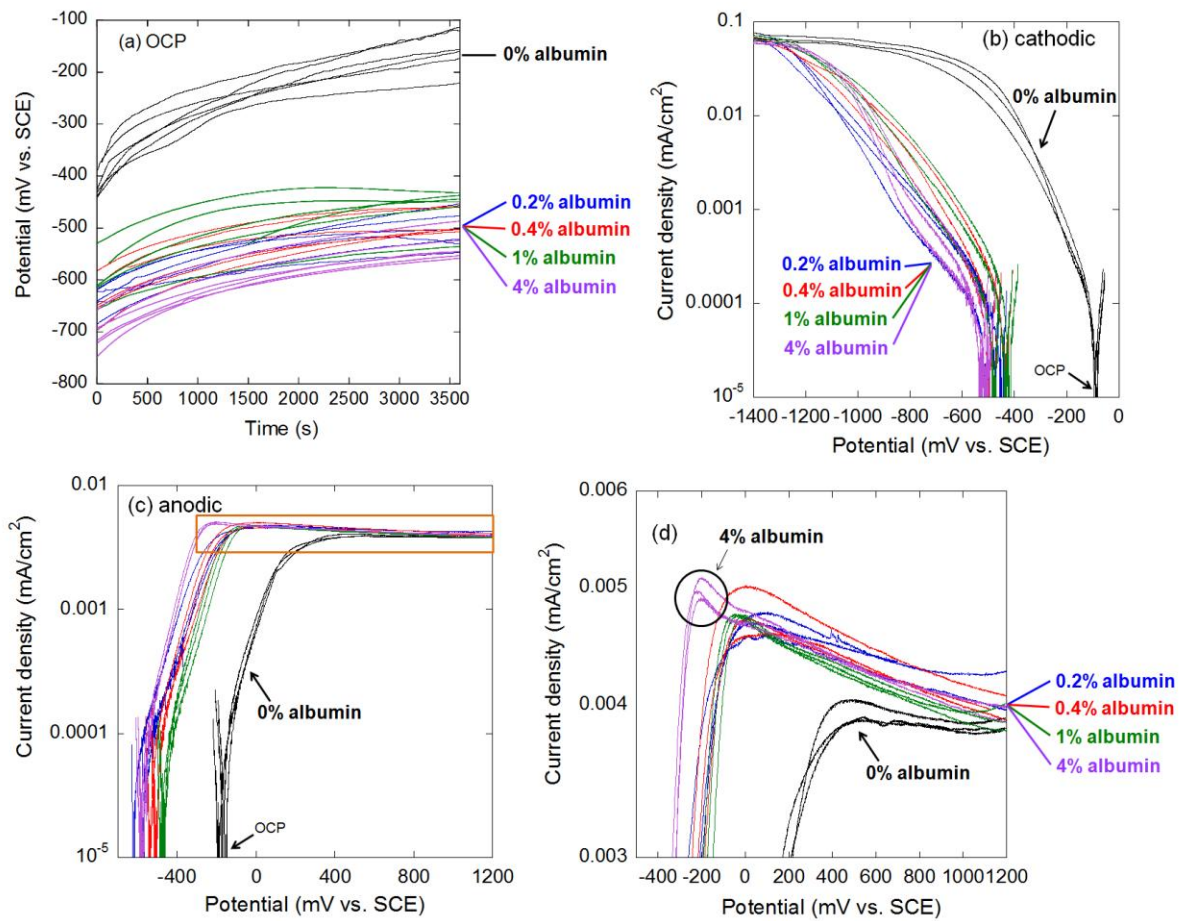


Figure 4 (a) OCP as a function of time; (b) cathodic and (c) anodic polarisation curves; (d) enlarged image of the region outlined in (c) for mirror-polished Ti6Al4V in physiological saline (0.15 M NaCl) in the presence and absence of different levels of albumin at 37 °C. The sweep rate was 1 mV/s.

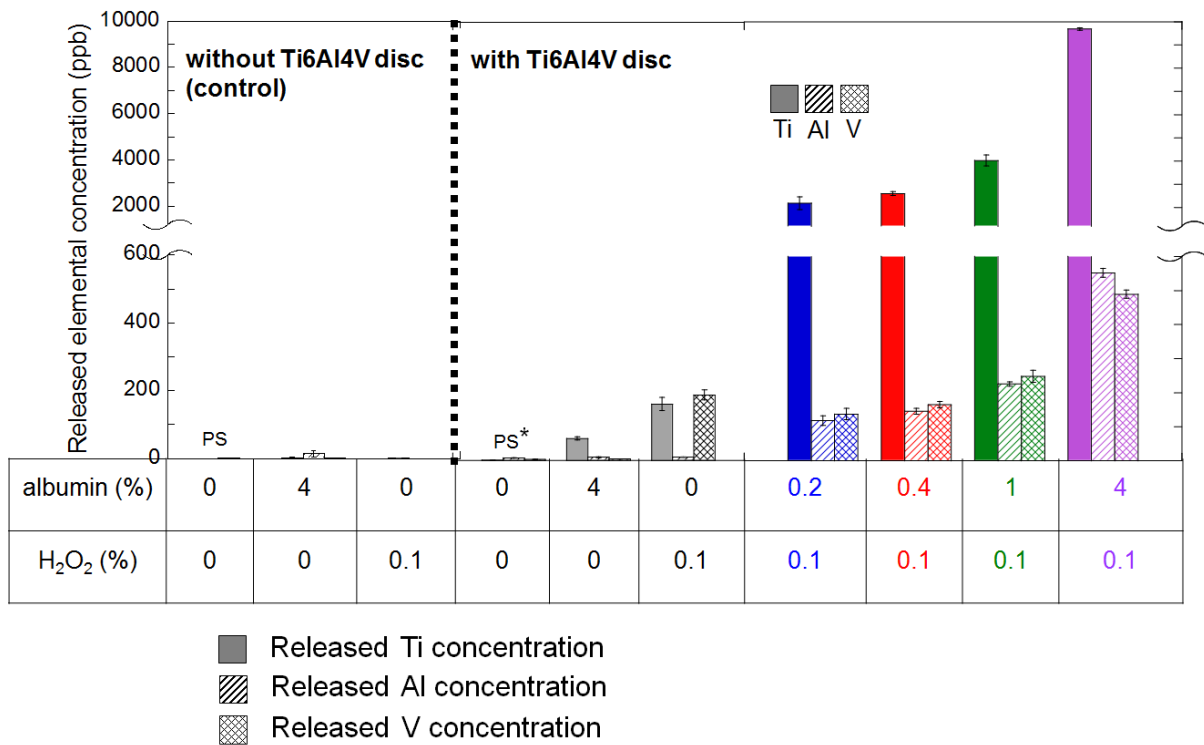


Figure 5 The mean concentrations and standard deviations (ppb) measured with ICP-MS of Ti, Al and V released from mirror-polished Ti6Al4V following immersion in physiological saline (PS, 0.15 M NaCl) with and without H<sub>2</sub>O<sub>2</sub> and albumin for 2 weeks at 37 °C (n=3); the results indicated \* were from 4 week immersion test shown in Figure 1.



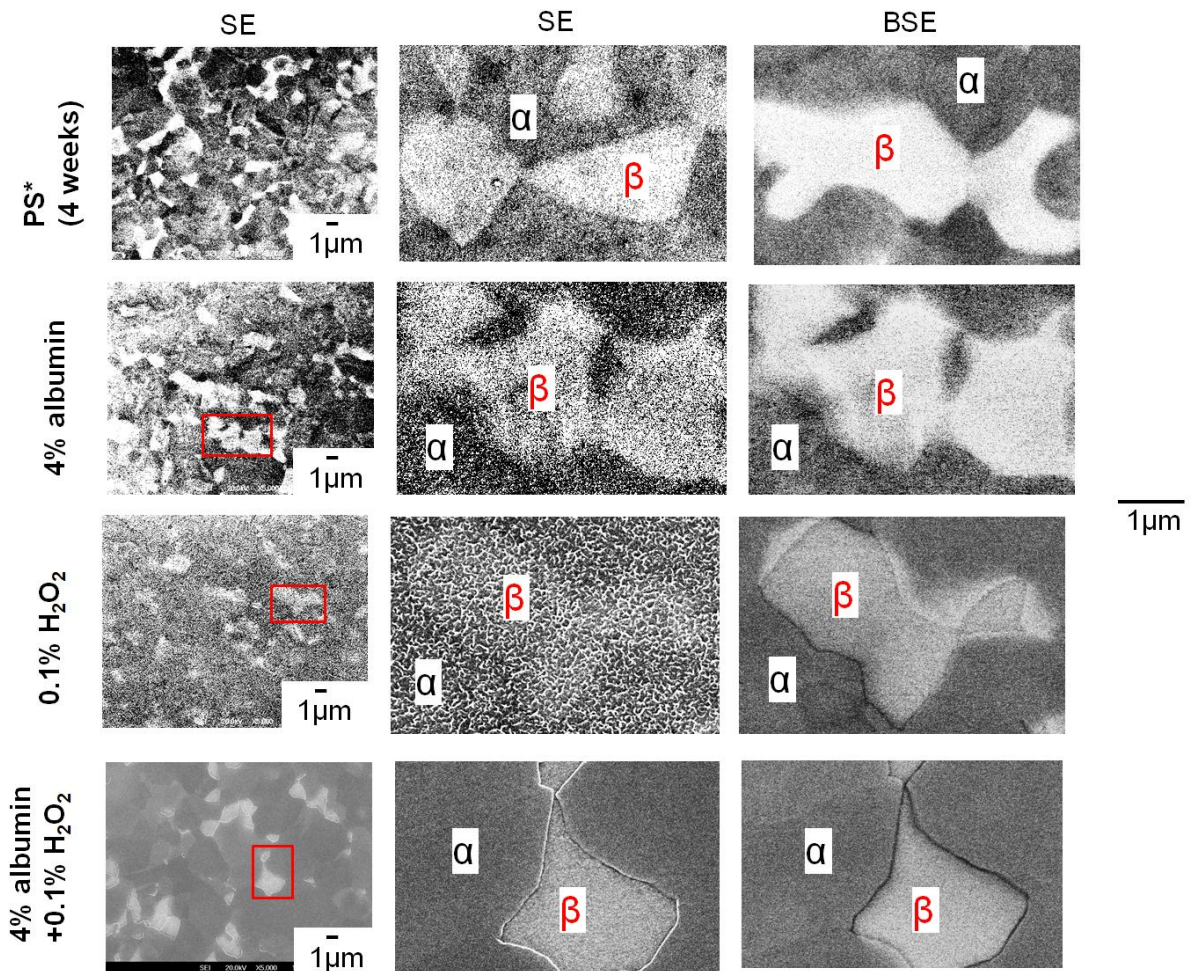


Figure 6 Surface morphology of mirror-polished Ti6Al4V following 2 week immersion in physiological saline (PS, 0.15 M NaCl) with or without H<sub>2</sub>O<sub>2</sub> and/or albumin at 37 °C; the results indicated \* were from the 4 week immersion test. SE: secondary electron SEM image; BSE: backscatter electron SEM image.


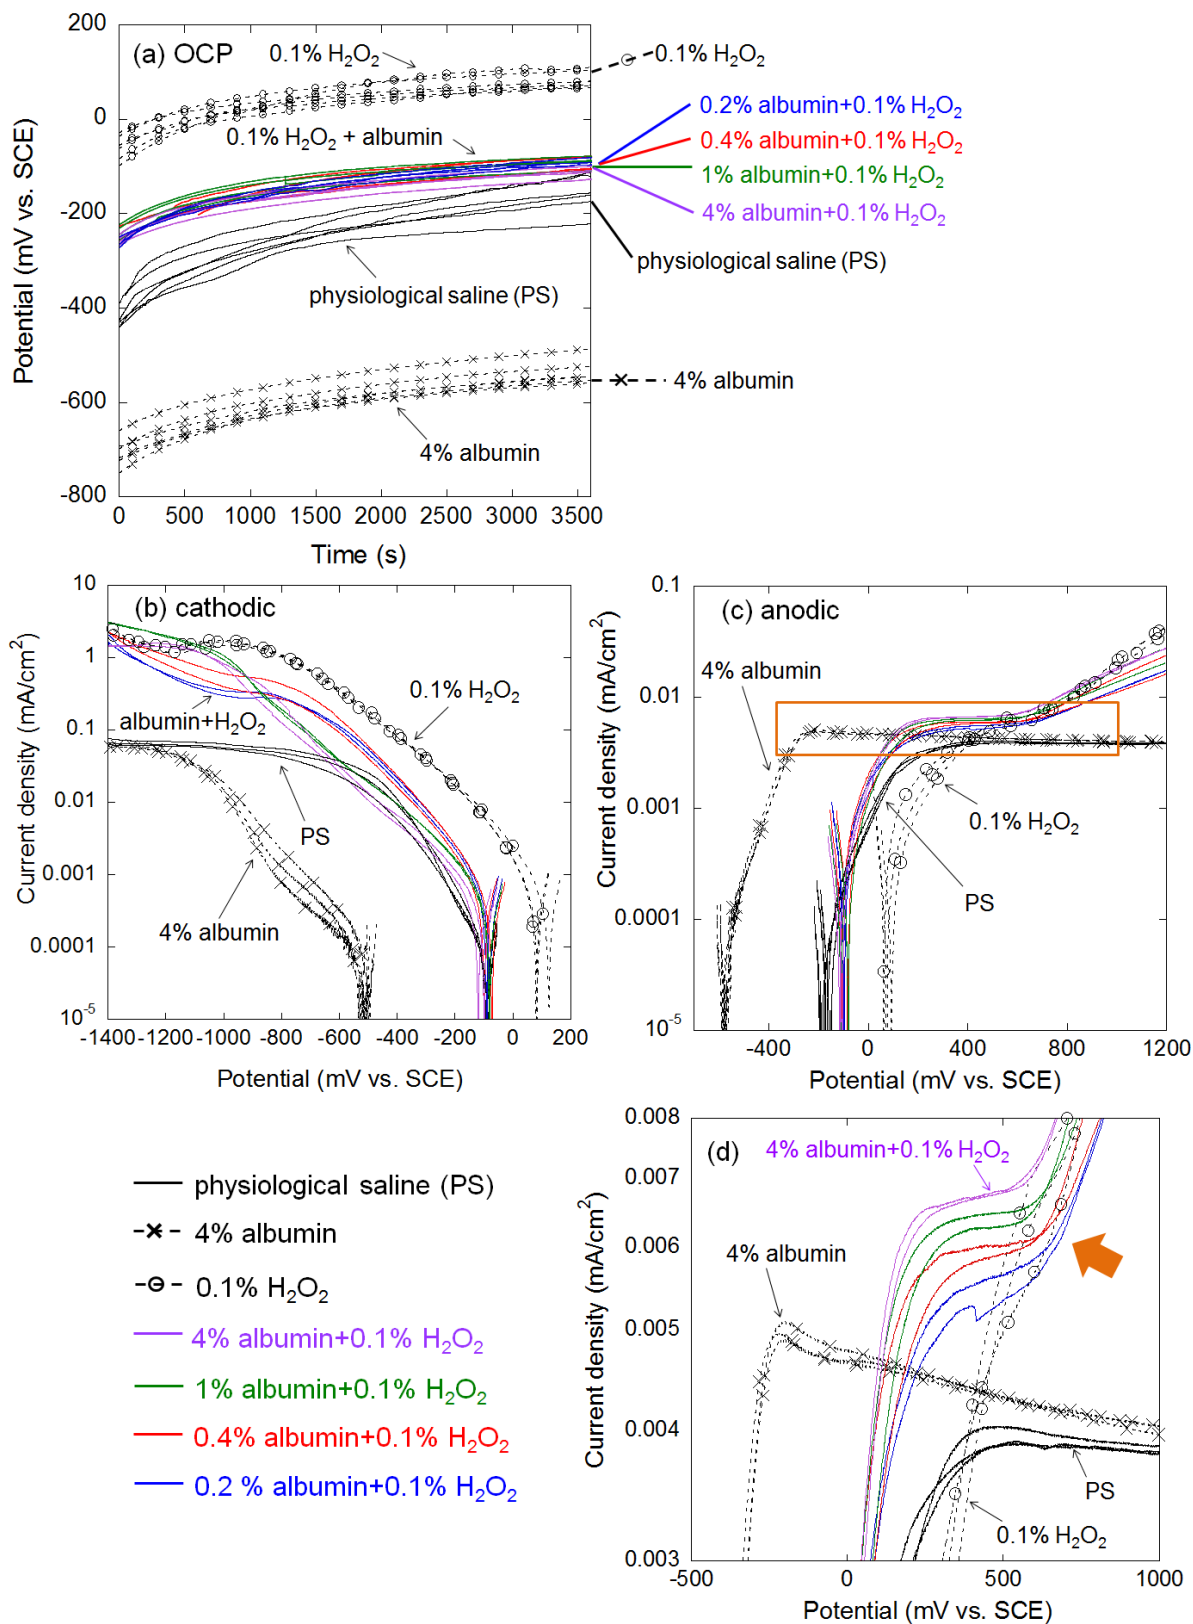


Figure 7 (a) OCP as a function of time; (b) cathodic and (c) anodic polarisation curves; (d) enlarged image of the region outlined in (c) for mirror-polished Ti6Al4V in physiological saline (PS, 0.15 M NaCl) with and without H<sub>2</sub>O<sub>2</sub> and different levels of albumin at 37 °C. The sweep rate was 1 mV/s.



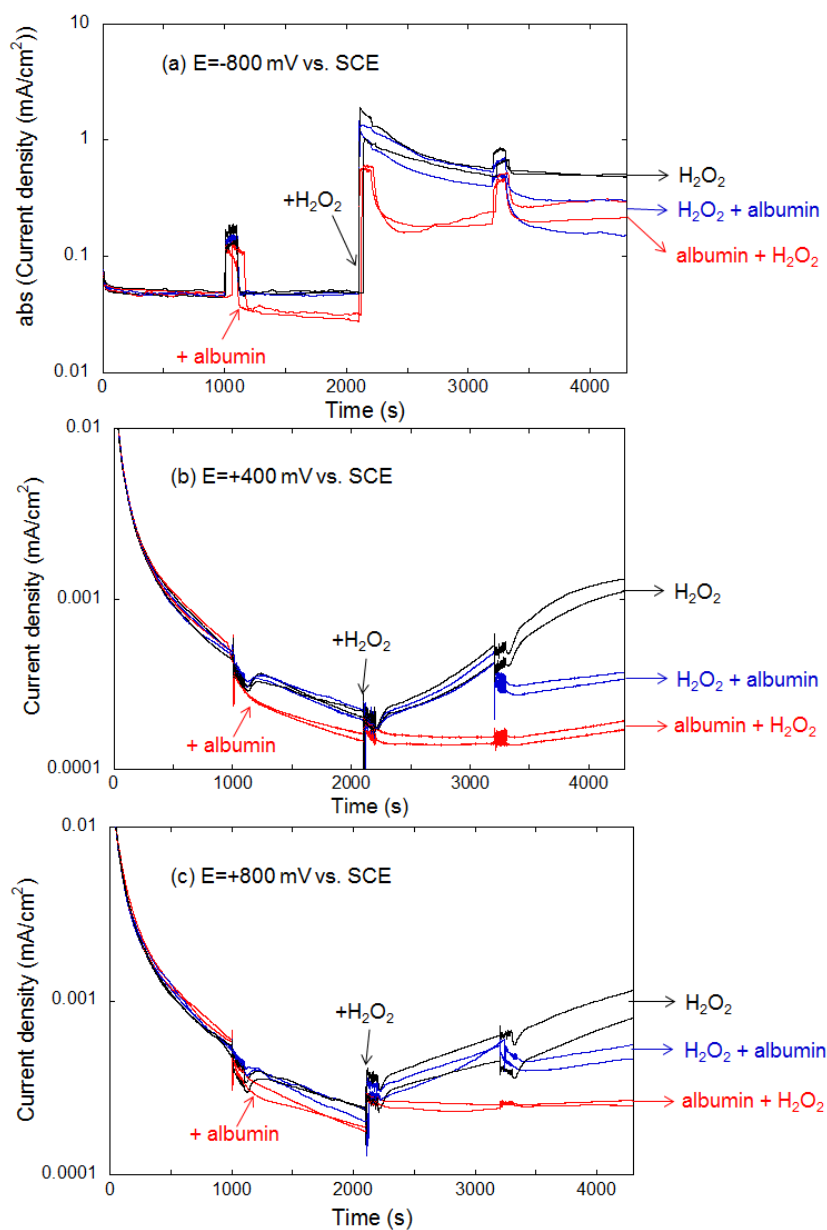

1st ~1000s	100s stir	2nd ~1000s	100s stir	3rd ~1000s	100s stir	1000s
PS	+1% albumin		+0.1% H <sub>2</sub> O <sub>2</sub>			
PS			+0.1% H <sub>2</sub> O <sub>2</sub>		+1% albumin	
PS			+0.1% H <sub>2</sub> O <sub>2</sub>			

Figure 8 Potentiostatic measurements of mirror-polished Ti6Al4V at (a) -800 mV; (b) 400 mV and (c) 800 mV vs. SCE in physiological saline (PS, 0.15 M NaCl) with addition of H<sub>2</sub>O<sub>2</sub> and/or albumin at 37°C. The solution was stirred for ~100 s at ~1000 s intervals to ensure complete mixing; for some experiments, a specific amount of H<sub>2</sub>O<sub>2</sub> or albumin (in PS) was added at ~1000 s intervals immediately before stirring to give a final concentration of 0.1% or 1%.

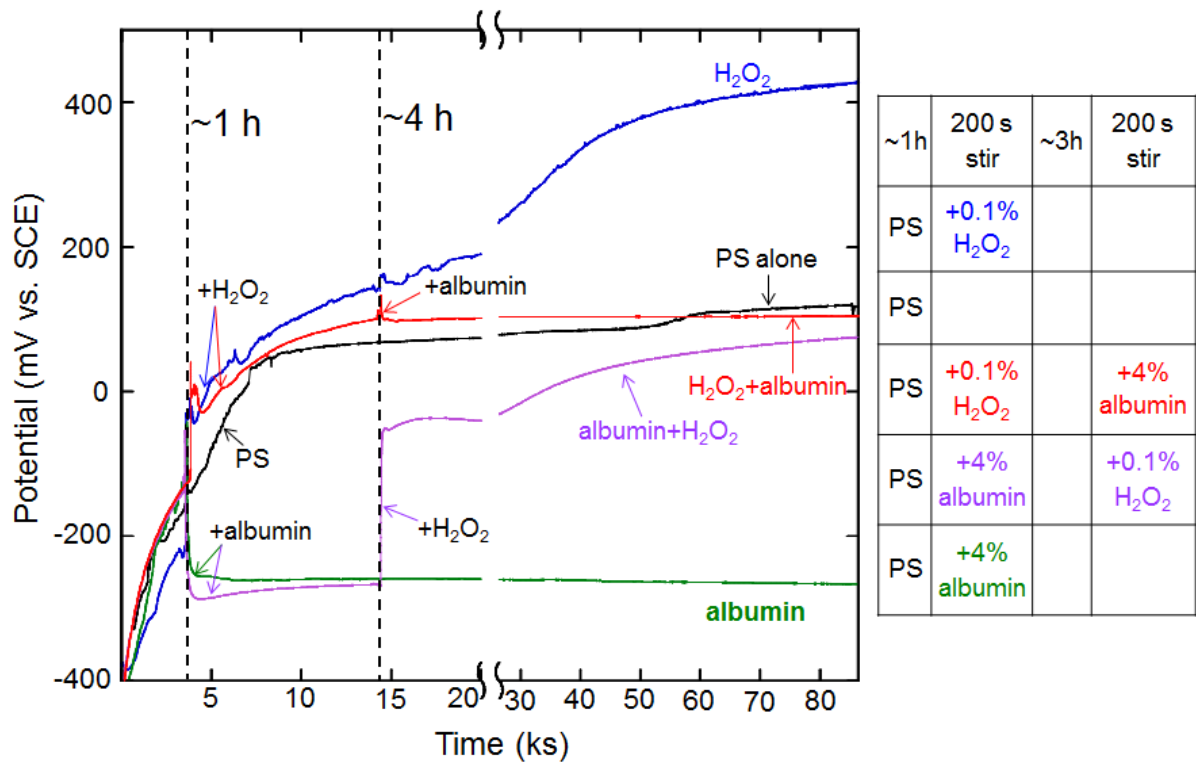


Figure 9 OCP as a function of time for 24 h for mirror-polished Ti6Al4V in physiological saline (PS, 0.15 M NaCl) with and without addition of H<sub>2</sub>O<sub>2</sub> and/or albumin at 37 °C. The solution was stirred for ~200 s at ~1 h and ~4 h to ensure complete mixing; for some experiments, a specific amount of H<sub>2</sub>O<sub>2</sub> or albumin (in PS) was added at ~1 h or ~4 h immediately before stirring to give a final concentration of 0.1% or 4%.

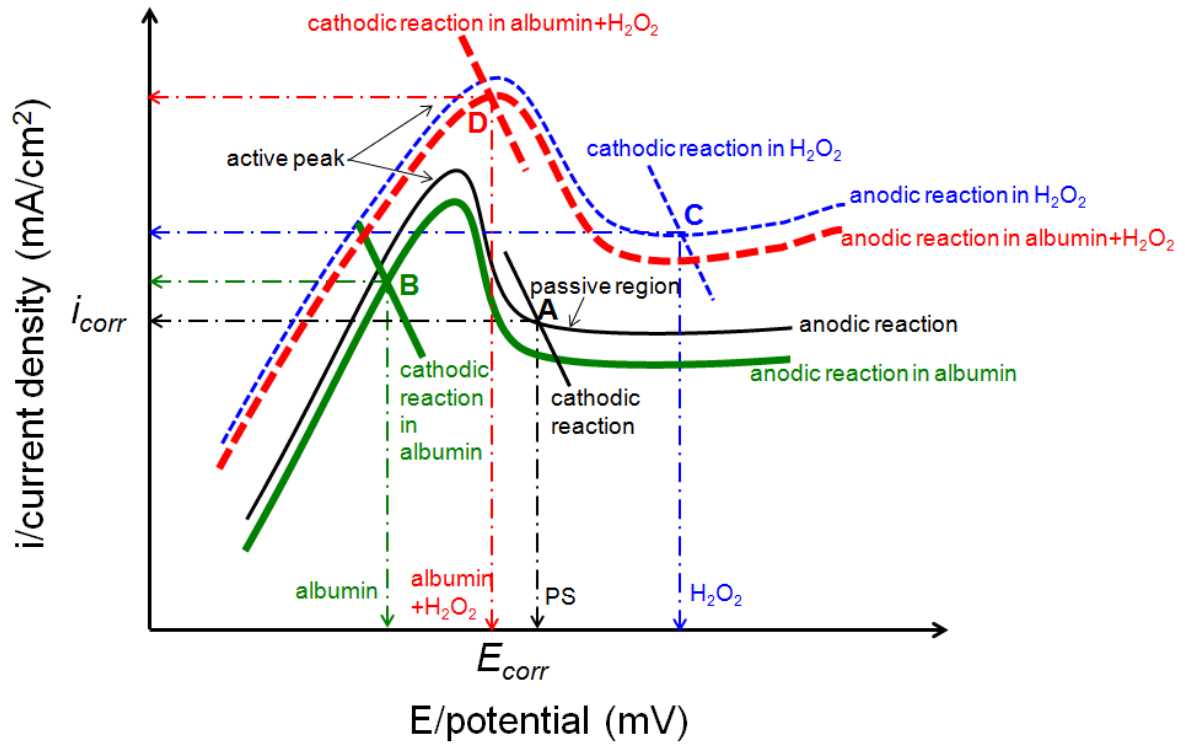


Figure 10 Schematic Evans diagram (mixed potential theory) to show the effect of H<sub>2</sub>O<sub>2</sub>, albumin and the combination of albumin and H<sub>2</sub>O<sub>2</sub> on corrosion potential ( $E_{corr}$ ) and corrosion current density ( $i_{corr}$ ) of Ti6Al4V in physiological saline (PS).