

# The Curse of Big Data in Diffuse Optical Spectroscopic Tomography: The LUCA approach

Dehghani, Hamid; Wojtkiewicz, Stanislaw

## *Document Version*

Early version, also known as pre-print

## *Citation for published version (Harvard):*

Dehghani, H & Wojtkiewicz, S 2020, The Curse of Big Data in Diffuse Optical Spectroscopic Tomography: The LUCA approach. in *Biophotonics Congress: Biomedical Optics 2020 (Translational, Microscopy, OCT, OTS, BRAIN)*. Optical Society of America.

[Link to publication on Research at Birmingham portal](#)

## **General rights**

Unless a licence is specified above, all rights (including copyright and moral rights) in this document are retained by the authors and/or the copyright holders. The express permission of the copyright holder must be obtained for any use of this material other than for purposes permitted by law.

- Users may freely distribute the URL that is used to identify this publication.
- Users may download and/or print one copy of the publication from the University of Birmingham research portal for the purpose of private study or non-commercial research.
- User may use extracts from the document in line with the concept of 'fair dealing' under the Copyright, Designs and Patents Act 1988 (?)
- Users may not further distribute the material nor use it for the purposes of commercial gain.

Where a licence is displayed above, please note the terms and conditions of the licence govern your use of this document.

When citing, please reference the published version.

## **Take down policy**

While the University of Birmingham exercises care and attention in making items available there are rare occasions when an item has been uploaded in error or has been deemed to be commercially or otherwise sensitive.

If you believe that this is the case for this document, please contact [UBIRA@lists.bham.ac.uk](mailto:UBIRA@lists.bham.ac.uk) providing details and we will remove access to the work immediately and investigate.

# The Curse of Big Data in Diffuse Optical Spectroscopic Tomography: The LUCA approach

Hamid Dehghani and Stanislaw Wojtkiewicz

*School of Computer Science, College of Engineering and Physical Sciences, University of Birmingham, Edgbaston, B15 2TT, UK*

*Author e-mail address: h.dehghani@cs.bham.ac.uk*

**Abstract:** NIR technologies now allow large scale data capture; therefore, computational and image recovery tools face new challenges to allow accurate and real-time applications. Key significant advancements as developed under NIRFAST will be presented together with clinical examples.

©2020 Optical Society of America

**OCIS codes:** (100.3190) Inverse problems; (170.3660) Light propagation in tissues;

## 1. Introduction

The development of Near Infrared (NIR) optical tomography and spectroscopic (NIRS) imaging as a functional imaging modality has relied largely on the use of model based image reconstruction. The recovery of optical parameters (inverse problem), namely spectrally varying absorption and scatter based parameters, from limited number of discrete boundary measurements of light propagation within tissue is inherently a difficult one as (1) Non-linearity means that a change in optical parameters does not provide an equal or linear change in the measured data, (2) Ill-posedness meaning that if a solution exists it may not be unique and its behavior does not change continuously with the initial conditions (3) Ill-conditioned such that a small change in measured data maybe due to a large change in optical parameters and (4) Under-determined as there are often many more parameters to be recovered than there are measured data. The continued development of the technology to date has made a substantial contribution towards providing more information regarding the tissue being imaged either through sophisticated systems that provide many more sets of data (Intensity, Phase, Time-of-Flight, Speckle, Luminescence to name a few) as well as systems that combine multiple-modalities (such as Ultrasound, CT, MRI) to help better constrain the problem as well as providing complementary functional data. The challenge from a model-based analysis then becomes how to incorporate these large sets of data, in a computational efficient manner, which is useful, accurate and meaningful.


To demonstrate the utilization of large sets of data, the LUCA project is used as an example, with specific emphasis on the novel numerical modeling approach of light propagation in tissue (such as spectral deconvolution, self-calibrating spectral Time Resolved data, data-reduction) as well as image reconstruction (single-step for NIRS and DCS, utilization of multi-modal data, structural and spectral priori) using boundary data using large sets of single and multi-modality data. Specific details regarding the creation, utilization and validation of these novel and sophisticated numerical models, as well as detail of the basis for using spatial and structural prior information will be outlined, together with phantom and patient data, whereby the use of spectral and dual-modality systems can improve contrast and spatial resolution. This work will demonstrate and highlight that the utilization of Big Data, if implemented correctly, is useful and does overcome the constrains of traditional diffuse tomography.

## 2. Methods

A system has been developed as a standalone tool for recovery of human thyroid hemodynamic parameters and is configured to utilize data from three complimentary diagnostic techniques: multi-spectral time resolved spectroscopy (TRS) [1] to measure concentrations of tissue constituents, diffuse correlation spectroscopy (DCS) [2] to assess perfusion and ultrasound images (US) for optical probes positioning and developing the tissue computational model.

## 3. Results

The thyroid parameters recovery as implemented in the LUCA device is shown in Fig.1. A cloud-based system (NIRFAST) has been tested within the LUCA device environment and phantom data. Execution time of the recovery procedure is <120s and marginally increases if multiple parallel examinations are processed with the parameter recovery algorithm as used in the LUCA device tested on in-vivo patient data [3]. Data were measured on 4 points above thyroid and 2 reference points outside. The TRS data were measured at 3 wavelengths (690, 785 and 830 nm) with the recovered hemodynamic thyroid parameters are shown in Fig. 1.

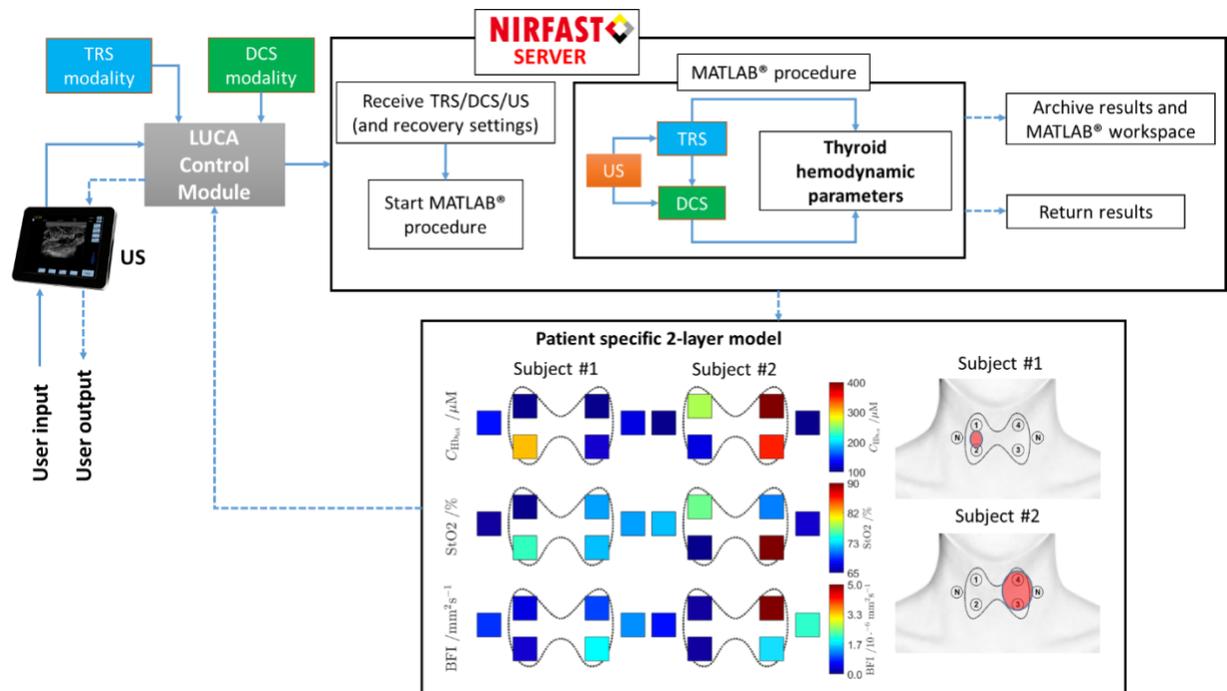

**Figure 1.** Thyroid parameters recovery as implemented in the LUCA system. Malignant lesions and measurement points locations are overlaid on the neck images. TRS – time resolved spectroscopy, DCS – diffuse correlation spectroscopy, US – ultrasound,  $C_{HbTot}$  – total haemoglobin concentration,  $StO_2$  – tissue perfusion index, BFI – blood flow index (perfusion index).

#### 4. Discussions and Conclusions

The model-based tissue parameters recovery has been implemented as a standalone tool within the LUCA thyroid cancer screening system. Modular architecture and remote access through TCP/IP protocol make the server a universal tool, which can be utilized for a wide range of biomedical optics applications as a post-processing box within an instrument, a WWW-based calculation service with e.g. a web interface or as a laboratory calculation server where researchers can operate on remote NIRFAST instances directly from their own MATLAB® copy. A number of new developments to allow fast real-time implementation of model-based parameter recovery have been utilized, such as self-calibrating algorithms [4], spectral deconvolution of Time Resolved NIRS data [5] and GPU implementation of the forward solver to dramatically enhance computational time [6]. This work has demonstrated and highlighted that the utilization of Big Data, if implemented correctly is useful and does overcome the constraints of traditional diffuse tomography.

#### 5. Funding

This work has received funding from the European Union's Horizon 2020 research and innovation programme under grant agreement No 688303. We acknowledge useful discussions with all consortium members.

#### 6. References

1. Sekar, S.K.V., et al., *Broadband (600-1350 nm) Time-Resolved Diffuse Optical Spectrometer for Clinical Use*. Ieee Journal of Selected Topics in Quantum Electronics, 2016. **22**(3).
2. Durduran, T. and A.G. Yodh, *Diffuse correlation spectroscopy for non-invasive, micro-vascular cerebral blood flow measurement*. Neuroimage, 2014. **85**: p. 51-63.
3. Lindner, C., et al., *Diffuse Optical Characterization of the Healthy Human Thyroid Tissue and Two Pathological Case Studies*. Plos One, 2016. **11**(1).
4. Wojtkiewicz, S., et al., *Self-calibrating time-resolved near infrared spectroscopy*. Biomedical Optics Express, 2019. **10**(5): p. 2657-2669.
5. Wojtkiewicz, S., T. Durduran, and H. Dehghani, *Time-resolved near infrared light propagation using frequency domain superposition*. Biomedical Optics Express, 2018. **9**(1): p. 41-54.
6. Doulerakis, M., et al., *Toward real-time diffuse optical tomography: accelerating light propagation modeling employing parallel computing on GPU and CPU*. Journal of Biomedical Optics, 2017. **22**(12).